

Proceedings

EXPERIENCING LIGHT 2009

International Conference on the Effects of Light on Wellbeing

Y. A. W. de Kort, W. A. IJsselsteijn, I. M. L. C. Vogels,
M. P. J. Aarts, A. D. Tenner, & K. C. H. J. Smolders (Eds.)

Keynotes and selected full papers
Eindhoven University of Technology,
Eindhoven, the Netherlands, 26-27 October 2009

Volume Editors

Yvonne de Kort, PhD

Wijnand IJsselsteijn, PhD

Karin Smolders, MSc

Eindhoven University of Technology

IE&IS, Human-Technology Interaction

PO Box 513, 5600 MB Eindhoven, The Netherlands

E-mail: {y.a.w.d.kort, w.a.ijsselsteijn, k.c.h.j.smolders}@tue.nl

Ingrid Vogels, PhD

Visual Experiences Group

Philips Research

High Tech Campus 34, WB 3.029

5656 AE Eindhoven, The Netherlands

E-mail: ingrid.m.vogels@philips.com

Mariëlle Aarts, MSc

Eindhoven University of Technology

Department of Architecture Building and Planning

PO Box 513, VRT 6.34

5600 MB Eindhoven, The Netherlands

E-mail: M.P.J.Aarts@tue.nl

Ariadne Tenner, PhD

Independent consultant

Veldhoven, The Netherlands

E-mail: ariadne.tenner@onsmail.nl

ISBN: 978-90-386-2053-4

Copyright:

These proceedings are licensed under Creative Commons Attribution 3.0 License (Noncommercial-No Derivative Works) This license permits any user, for any noncommercial purpose – including unlimited classroom and distance learning use – to download, print out, archive, and distribute an article published in the EXPERIENCING LIGHT 2009 Proceedings, as long as appropriate credit is given to the authors and the source of the work.

You may not use this work for commercial purposes. You may not alter, transform, or build upon this work.

Any of the above conditions can be waived if you get permission from the author(s).

For any reuse or distribution, you must make clear to others the license terms of this work.

The full legal text for this License can be found at

<http://creativecommons.org/licenses/by-nc-nd/3.0/us/legalcode>

Reference specification:

Name Author(s), “Title of the Article”, In: Proceedings of EXPERIENCING LIGHT 2009 International Conference on the Effects of Light on Wellbeing (Eds. Y.A.W. de Kort, W.A. IJsselsteijn, I.M.L.C. Vogels, M.P.J. Aarts, A.D. Tenner, and K.C.H.J. Smolders), 2009, pp. X (startpage) – Y (endpage).

Ecological Measurements of Light Exposure, Activity, and Circadian Disruption in Real-world Environments

Daniel Miller, MS,¹ Andrew Bierman, MS,¹ Mariana G. Figueiro, PhD,¹
Eva S. Schernhammer, MD, DrPH,² Mark S. Rea, PhD¹

¹ **Lighting Research Center**
Rensselaer Polytechnic Institute
21 Union Street
Troy, NY 12180 USA
+1 518 687-7100
ream@rpi.edu

² **Brigham and Women's Hospital and
Harvard Medical School**
Channing Laboratory, 3rd Floor
181 Longwood Avenue
Boston, MA 02115 USA
+1 617 525-4648

ABSTRACT

Presented is an overview of the recently developed Daysimeter, a personal measurement device for recording activity and circadian light-exposure. When the Daysimeter is worn on the head, two light sensors near the eye are used to estimate circadian stimulus (CS_A) exposures over extended periods of time. Phasor analysis combines the measured periodic activity-rest patterns with the measured periodic light-dark patterns to assess behavioral circadian entrainment/disruption. As shown, day-shift and rotating-shift nurses exhibit remarkably different levels of behavioral circadian entrainment/disruption. These new ecological measurement and analysis techniques may provide important insights into the relationship between circadian disruption and well-being.

Keywords

Circadian rhythms, phasor analysis, circadian disruption, Daysimeter, circadian light, phototransduction

INTRODUCTION

The synchronization of the endogenous master clock to local time on earth is governed by a robust and regular 24-hour pattern of light and dark on the retina. If the light-dark pattern is not above threshold, or if its period is something other than 24-hours, human biology is disrupted, from single cells to overt behavior [6, 14]. Circadian disruption can manifest itself in poor sleep, digestion, reduced attention and performance [8, 9, 15]. Over time this disruption can lead to serious maladies such as cardiovascular disease [24], diabetes and obesity [1], and cancer [17, 19, 20]. Despite the plethora of animal and epidemiological research demonstrating the negative impact of circadian disruption on health, surprisingly little is known about the levels of circadian disruption actually experienced by people in different types of living conditions and environments.

This paper describes a measurement tool for collecting ecological data on circadian light-dark stimuli and rest-activity patterns along with methods of analyzing such data so that circadian entrainment and disruption can be assessed. Results of using such techniques to study a cohort of nurses engaged in both day- and rotating-shift work is also presented.

INSTRUMENTATION

The Daysimeter™ was developed as a personal circadian light exposure and activity meter to measure circadian light-dark and activity-rest patterns in the field [3]. It was necessary to develop a sophisticated, small photometer calibrated in terms of the spectral-spatial-intensity response of the human circadian system. Moreover, since light must be incident on the retina to be effective, the Daysimeter had to be designed to place the light sensors near the plane of one cornea. Extending from a number of basic studies on circadian phototransduction [2, 4, 21], and physiological optics [22], a model was developed for human circadian phototransduction [12], and this model forms the basis of the Daysimeter's photometric response characteristics. To measure activity, the Daysimeter incorporates accelerometers that respond to head movements and orientation with respect to Earth's gravitational field. Activity and light are measured together at regular time intervals and electronically stored. In addition, the Daysimeter logs its operating temperature. Using practical power management techniques, the Daysimeter can gather light, activity and temperature data for up to 30 days for subsequent analysis.

Two calibrated photosensors are employed to measure optical radiation in close proximity to the cornea. Based upon the spatial sensitivity model of the retina developed by Van Derlofske et al. [22], both sensors have a nearly cosine spatial response meaning that the sensors are most sensitive to light at normal incidence with sensitivity at

other angles decreasing proportional to the cosine of the incident angle. One sensor is a conventional glass-filtered silicon photodiode (Hamamatsu model S1286, custom glass filter) having a spectral sensitivity closely matching the standard photopic luminous efficiency function, $V(\lambda)$ [5]. The other sensor is a short-wavelength (blue) sensor fabricated from a gallium arsenide phosphide (GaAsP) photodiode (Hamamatsu model GA5645), having an intrinsic long wavelength response cutoff at approximately 580 nm, together with a UV blocking glass filter (Schott GG395). This “blue” sensor has a spectral response peaking at approximately 460 nm with an 80 nm full-width-half-maximum (FWHM) bandpass.

Once the optical radiation data obtained by the Daysimeter from both sensors are downloaded to a computer, “circadian light” levels can be approximated using post-processing algorithms based upon the model of circadian phototransduction by Rea et al. [12]. The values of circadian light levels are scaled so that 1000 lux of CIE Illuminant A (an incandescent blackbody radiator at 2856 K) is equivalent to 1000 circadian light units (CL_A). Four spectral sensitivity functions are used in the model: the scotopic luminous efficiency function, $V'(\lambda)$ [5], based on rod sensitivity, $V_{10}(\lambda)$ based upon the S, M and L cone fundamentals [16], the S-cone fundamental [18], and a standard photo-opsin emulating melanopsin contained within the intrinsically photosensitive retinal ganglion cell (ipRGC; [2]) and having a peak spectral response at 480 nm and a half-bandwidth of 95 nm. Briefly, in the model the cone fundamentals form a spectrally opponent (blue vs. yellow [7]) input to the ipRGC which sends circadian light signals to the SCN. The modeled rod response suppresses output from the ipRGC when the blue-yellow opponent signal is positive, with diminishing suppression at higher irradiance levels as rods become more fully bleached. A negative blue-yellow opponent signal, however, produces a response determined solely by the ipRGC (no cone input and no rod suppression). The Daysimeter system uses its two spectral channels to approximate the four spectral channel input in the model. Discrepancies were minimized between the two-channel estimates and the four-channel model calculation of CL_A for several practical light sources using a conventional least-squares technique. Based upon those results, algorithms were developed to minimize measurement errors of CL_A from the Daysimeter; the results of that analysis are shown in Figure 1. Spectral mismatch errors of the photopic channel for the light sources in Figure 1 are less than 2% except for the 470 nm LED which has a photopic spectral mismatch error of 8%.

The human circadian system response to light (CL_A), as measured by acute nocturnal melatonin suppression [10], follows a logistic function [25]. This response function is used to transform the CL_A values into circadian stimulus values (CS_A). CS_A is considered to be a better measure of the effectiveness of the light stimulus for the human circadian system because it is defined in terms of the

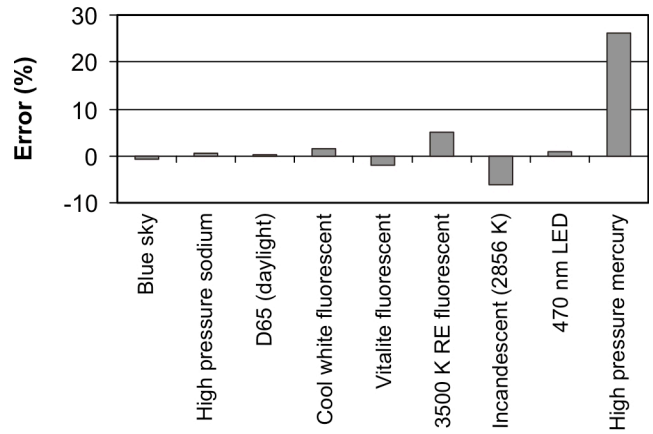


Figure 0. Errors in estimating a fixed level of circadian stimulus (1000 CL_A) from the model of circadian phototransduction by Rea et al. [12] generated by several common light sources using the algorithms applied to the two-sensor data acquired by the Daysimeter.

circadian system’s input-output relationship, including both threshold and saturation.

The Daysimeter model used in the present study had two orthogonally oriented accelerometers contained within a single electronic sensor package (Analog Devices, model number ADXL330) and mounted on the Daysimeter’s circuit board. The outputs of the sensor package are voltages that are proportional to the instantaneous acceleration of each accelerometer. These voltages are converted to digital values using the 12-bit analog-to-digital converter of the microprocessor (Texas Instrument MSP430F169) that controls operation of the Daysimeter. The digital data are acquired once per second, and then used to calculate an activity index every 30 s using the following equation:

$$\text{Activity Index} = k \sqrt{\frac{(SS_x + SS_y)}{n}}$$

where SS_x and SS_y are the sums of the squared deviations from the mean digital value for each accelerometer (x and y) over the 30-second logging interval, n is the number of samples (30), and k is a calibration factor converting the measured output voltage of the accelerometers in arbitrary analog-to-digital converter counts to units of g-force (1 g-force = 9.8 m/s²). In other words, the activity index is the root-mean-square (rms) deviation in acceleration in two dimensions measured for every 30-second logging interval.

ANALYSIS METHODS

Phasor analysis, a technique based on signal processing techniques [11], makes it possible to interpret the light and activity data, sampled together over consecutive multiple days (usually seven days for the data presented here), in terms of the phase and magnitude of the joint 24-hour patterns. The correlations between the periodic changes in light and in activity are first determined by calculating the circular correlation function of the light and activity time series. The circular correlation function reveals how the correlation (r , not r^2) between light and activity change as a

function of the timing difference, or phase between them (Figure 2). The circular correlation function is then decomposed into its temporal frequencies and phase angles using Fourier analysis techniques, from which the 24-hour frequency component is selected as a measure of circadian rhythmicity. The 24-hour phasor magnitude is used as the metric for behavioral circadian entrainment/disruption; the greater the magnitude, the greater the level of behavioral circadian entrainment of activity to light. The phasor angle reflects the phase relationship between the periodic light-dark exposure pattern and the periodic activity-rest pattern in the correlations (Figure 2). Figure 2 shows examples of

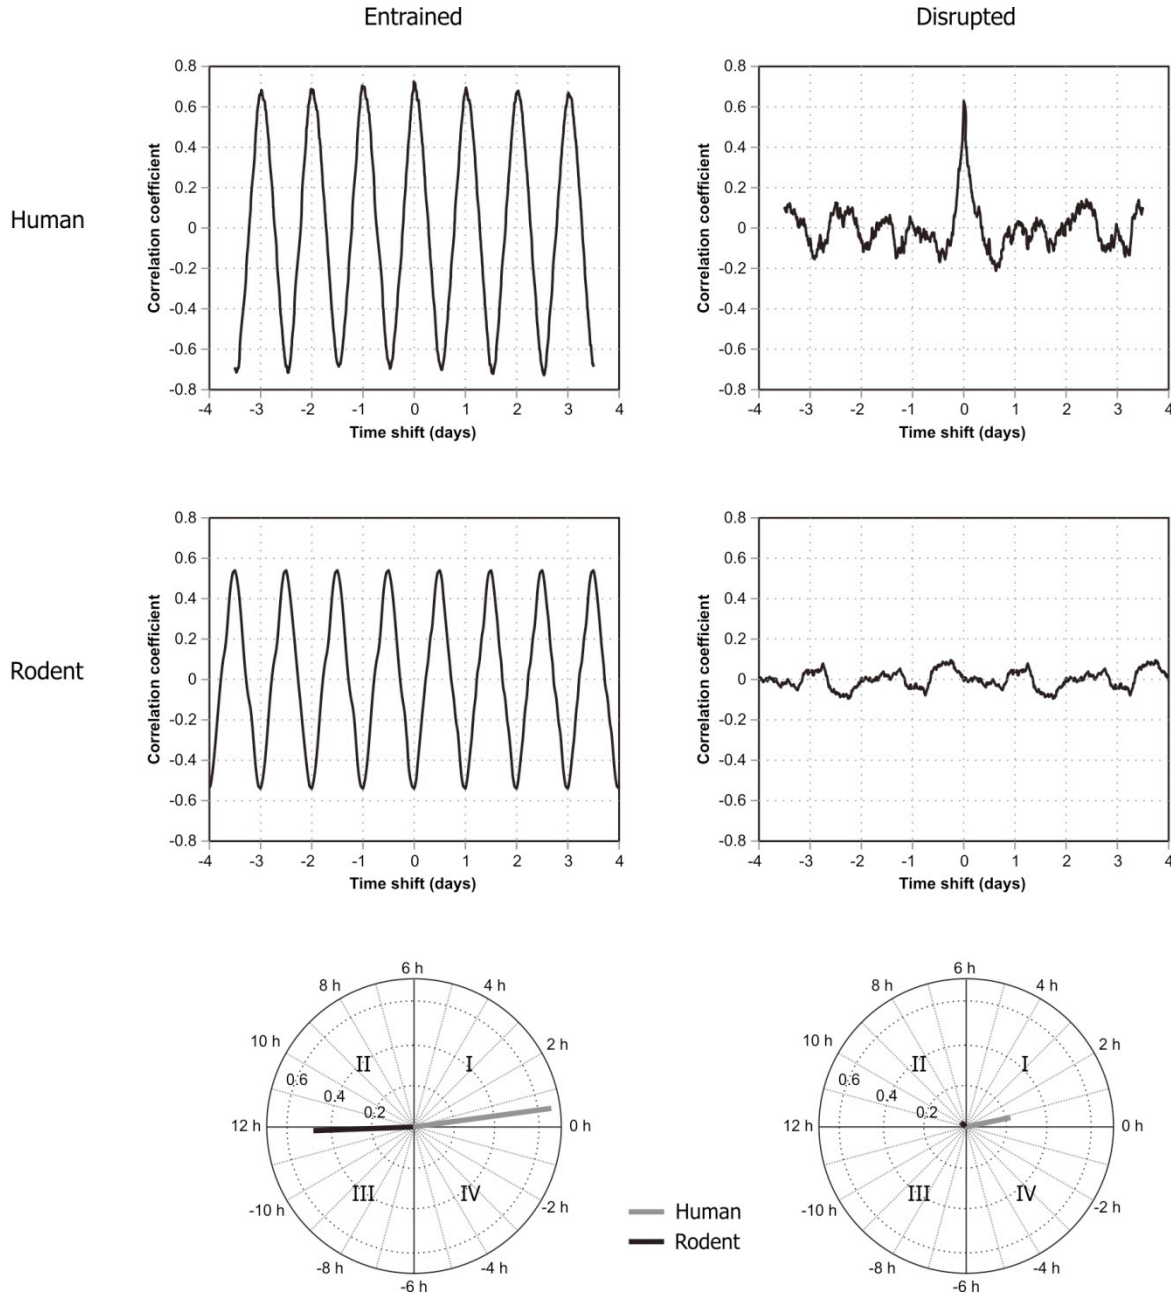


Figure 2: Circular correlation functions and associated phasors for two nurses, one day-shift and one rotating-shift, and for two nocturnal rodents, a rat exposed to a regular pattern of 12L:12D and a rat exposed to a “jet lag” pattern of light and dark (the 12L:12D pattern was reversed every 48 hours).

the circular correlation functions and associated phasors for two nurses, a day-shift nurse and a rotating-shift nurse, as well as for two nocturnal rodents, one exposed to a regular pattern of 12 hours light and 12 hours dark (12L:12D) and one exposed to a simulated “jet lag” pattern (discussed later in the text).

Two techniques of parsing the Daysimeter data can be used for phasor analysis. The “all-at-once” technique computes the circular correlation function of the entire data set (e.g., seven days) in one operation. The resulting circular correlation function provides the correlation coefficients between light and activity for time shifts in activity ranging from zero to the total length of time over which data were collected (usually seven days for the data collected here). Because the circular correlation extends over multiple days, this technique is sensitive to day-to-day variations as well as variations within each day. Fourier analysis applied to the all-at-once circular correlation extracts the magnitude and the angle of the 24-hour component, separating it from the longer, infradian, and shorter, ultradian, variations. If the power in these longer or shorter periods in the circular correlation is large, the magnitude of the 24-hour phasor is reduced. To facilitate Fourier harmonic analysis the time duration, or total length of the data set, is truncated to an integer number of days.

The “sliding-window” technique parses the data into a progression of overlapping 24-hour segments and calculates a circular correlation for every segment. Fourier analysis is applied to each of these circular correlation functions to extract the 24-hour, fundamental component. The resulting 24-hour phasors for each data segment are then averaged (vectorally) to arrive at a phasor representing the entire data collection period. The advantage of the sliding-window technique is that it utilizes all the available data without truncation; therefore, it is better than the all-at-once technique for short collection protocols because it utilizes all of the limited data available. A limitation of this technique, however, is that there is no ability with the sliding-window technique to identify rhythms slightly longer or shorter than 24 hours. Analyzing seven days of data using the all-at-once technique has a precision of approximately 3.4 hours for resolving the expressed circadian periods in the circular correlations, whereas the sliding-window technique cannot reliably resolve periods up to approximately 12 hours. This higher degree of period resolution with the all-at-once technique will necessarily result in shorter 24-hour phasor magnitudes than those obtained for the same data using the sliding-window phasors unless there is no significant power in the infradian or ultradian rhythms. This difference is most evident with disrupted subjects who do not necessarily show a strong 24-hour rhythm but still exhibit relatively large sliding-window phasor magnitudes. Because the period resolution is worse with the sliding-window technique than with the all-at-once technique, the power of the other non-24-hour periods also contribute to the phasor magnitude.

The activity index values can be used to compute two statistics developed by Van Someren et al. [23] to estimate the day-to-day consistency of activity over the recording session (interdaily stability, IS) and the hour to hour consistency of activity over the recording session (intradaily variability, IV). High values of IS indicate that the subject’s 24-hour activity and rest pattern was consistent over the entire recording session; high values of IV indicate that the subject’s pattern of activity and rest was highly fragmented with intermittent and inconsistent intervals of movement and no-movement. Neither statistic accounts for levels of light exposure or changes in light exposure levels.

DATA COLLECTION

The Nurses’ Health Study II is a prospective cohort study that began in 1989, when 116,671 registered female nurses in the United States between the ages 25 to 42 were enrolled. The study was designed to prospectively examine the effects of oral contraceptive use and other life style factors on chronic diseases, particularly cancers and cardiovascular diseases. Surviving nurses within this cohort were contacted to serve as potential subjects between November 2006 and April 2008; 138 nurses volunteered to participate. The study was approved by the Committees on the Use of Human Subjects in Research at the Brigham and Women’s Hospital and the Harvard School of Public Health, as well as Rensselaer’s Institute Review Board; written informed consent was obtained from each participant.

Reported here are results from Daysimeter measurements for 38 day-shift and 61 rotating-shift nurses; the rotating-shift nurses worked from one to five nights over the recording period. For 16 other nurses in the study who were categorized as rotating-shift, the Daysimeter data indicated that they did not work any nights during the study period, so their data are not included. The larger number of rotating-shift nurses reflects the initial assumption that day-shift nurses would be more homogenous with respect to circadian entrainment than the rotating-shift nurses. Data from 23 of the 138 nurses were unusable due to recording irregularities or non-compliance with the seven-day protocol. It was possible to identify data from those nurses who did not comply with the protocol by using the data from the Daysimeter’s on-board temperature sensor; room-temperature readings, as opposed to elevated temperatures when the Daysimeter is in close contact with the body, and extended periods of inactivity were certain signs that the nurse did not wear the device when required. Visual inspection of the temperature and activity data plotted against time was used to identify noncompliance. Only those protocol departures lasting about a day or more could be unambiguously identified and were removed. The data from 13 of the remaining 99 nurses showed non-compliance during only one to three days of the seven-day recording period. For these nurses, only the data for the noncompliant days were removed; 10 nurses provided six days of useful data and three provided five.

RESULTS

Table 1 summarizes the results of the measurements. Two-tailed student t-tests revealed that, on average, day-shift nurses were exposed to statistically higher levels of light (both photopic and CL_A) than rotating-shift nurses during the recording sessions. It is interesting to note, however, that the ratio of the average photopic light level to the average circadian level is similar for both day-shift and rotating-shift nurses. This suggests that the types of light sources, natural and electric, seen by both groups were not remarkably different for both groups. Interesting too, the average activity levels of the two groups were nearly identical. The phasor analysis of the continuous light and activity data provided by the Daysimeter indicated that the synchronization between the light-dark exposures and the

activity-rest behavior was much greater for the day-shift nurses than for the rotating-shift nurses based upon the highly significant difference between the two groups in terms of their respective phasor magnitudes determined using either the sliding-window or the all-at-once techniques. There was no difference between the two groups in terms of their phasor angles using the sliding-window technique, but there was a significant difference between the phasor angles of the two groups using the all-at-once technique. Following the earlier discussion, the all-at-once technique is much more sensitive to consistency in the light and activity patterns over the entire recording period than the sliding-window technique. Thus, there is a much larger difference between the two groups in terms of their phasor angles using the all-at-once technique.

Table 1.

	Photopic light (lux)	Circadian light (CL_A)	Activity Index ($\Delta g\text{-force}_{rms}$)	Interdaily Stability (IS)	Intradaily Variability (IV)	Phasors			
						Sliding-window		All-at-once	
						Magnitude	Angle (hours)	Magnitude	Angle (hours)
Day-shift (N=38)*	302 [188]	369 [227]	0.0094 [0.0014]	0.692 [0.144]	0.447 [0.170]	0.50 [0.11]	0.65 [0.74]	0.46 [0.12]	0.68 [0.71]
Rotating-shift (N=61)*	188 [152]	209 [166]	0.0097 [0.0018]	0.252 [0.129]	0.458 [0.135]	0.33 [0.10]	0.64 [0.73]	0.12 [0.10]	2.3 [3.2]
t-test p-value (two-tail)	0.0028	3.9×10^{-4}	0.26	2.1×10^{-24}	0.72	6.4×10^{-11}	0.94	2.7×10^{-24}	2.4×10^{-4}

* – Mean values shown; standard deviation values in [brackets].

Photopic light exposures: The Daysimeter system utilizes a fully calibrated (spectral, spatial, intensity) photopic light sensor measuring in lux (lm/m^2). Group means [standard deviation] are computed from individual subject means of each subject's entire recording session.

Circadian light exposures: Using the model from Rea et al. [12], circadian light exposure values are determined from the photopic and blue light sensor data measured in CL_A . Group means [standard deviation] are computed from individual subject means of each subject's entire recording session.

Activity index: Values from two orthogonally oriented accelerometers (measuring up/down and forward/back head motions) are used to compute an activity index that is logged at regular time intervals along with the light readings. Each logged measure of activity is the rms combination of the standard deviation of acceleration taken once per second over a 30-second interval of both accelerometers. Group means [standard deviation] are computed from individual subject means of each subject's entire recording session.

Interdaily stability: The IS statistic developed by Van Someren et al. [23] measures the consistency of activity among days and ranges from 0 to 1. A value of 1 results when every day's activity is identically to the other days, while conversely a value of 0 results from no similarity among days.

Intradaily variability: The IV statistic developed by Van Someren et al. [23] measures the fragmentation of rhythm between rest and activity based on a scale from 0 (no variability from hour to hour) to upwards of 2. A larger value indicates more fragmentation of rest and activity, or conversely, less consolidation of rest/activity patterns.

Phasor magnitude: A correlation between circadian light exposure and activity (calculated using either the sliding-window or the all-at-once technique) for the observation period, in this case 5-7 days. A higher magnitude indicates the subject has a consistent, 24-hour schedule with respect to activity and light. Lower magnitudes indicate low correlation between daily cycles of light and activity irrespective of phase differences.

Phasor angle: A phase relationship between circadian light exposure and activity (calculated using either the sliding-window or the all-at-once technique) for the observation period, in this case 5-7 days. A positive angle (first quadrant) indicates a delay in activity with respect to light and a negative angle (fourth quadrant) indicates an advance in activity with respect to

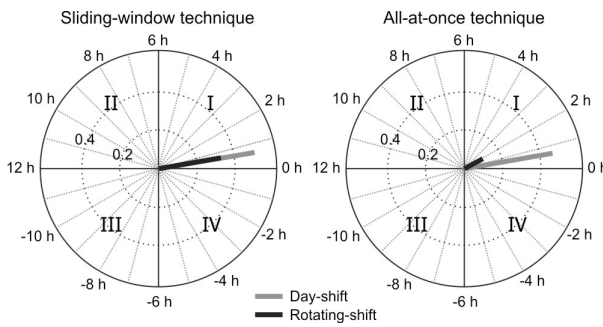


Figure 3. Average phasors for day-shift and for rotating-shift nurses using the sliding-window (left) and all-at-once (right) techniques. See text for discussion of the two methods.

Figure 3 illustrates on polar coordinates the average phasors for both groups using both techniques, sliding-window and all-at-once. For diurnal species the phasors typically plot in the first and fourth quadrants, indicating activity and light exposure are positively correlated. Phasor angles for humans are almost always in the first quadrant, indicating that activity is delayed with respect to light exposure, typically because people become active with the bright, morning light but continue to be active after sunset under dim, electric light; see later discussion on this point.

Figure 4 shows the distribution of the phasor magnitudes for the two groups of nurses on a linear scale, but broken down in terms of the number of night-shifts they worked during the recording period. Obviously the day-shift nurses did not work any nights; two rotating-shift nurses worked five nights. Figure 4 shows that, in general, as the number of working nights increase, phasor magnitudes decrease. This suggests that behavioral circadian disruption increases with the number of nights worked. It should be noted, however, that one of the two nurses who worked five nights had a higher phasor magnitude than all those working three or four nights and most working two nights, and that the highest average circadian disruption was for nurses working three night shifts during the week. This suggests that disruption might be less for people who continually work the night shift compared to those who do so

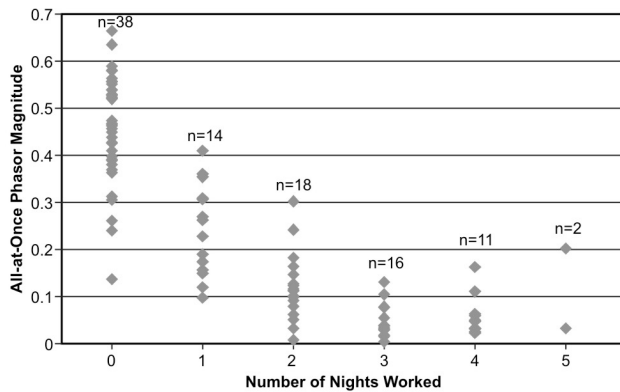


Figure 4: All-at-once phasor magnitudes for day-shift and rotating-shift nurses plotted as a function of the number of nights worked

intermittently, but, of course, there are too few samples to reach any reliable conclusions concerning the health of these nurses.

Figure 5 compares the sliding-window and the all-at-once techniques for computing phasor magnitudes for the day-shift and rotating-shift nurses. For the day-shift nurses, either method returns similar results ($r^2=0.91$). For the rotating-shift nurses, the similarity is reduced ($r^2=0.18$). The most obvious explanation being that the day-shift nurses are on a regular schedule with every day similar to every other day. Since their behavior conforms to a stable 24-hour pattern both techniques give the similar phasor magnitudes. Rotating-shift nurses, on the other hand, have variable schedules so they do not have stable 24-hour patterns of light and/or of activity. They exhibit a complex variety of rhythm periods, some slightly shorter and some longer than 24 hours. As previously discussed, the sliding-window technique lumps together a broader range of periods in the 24-hour phasor resulting in relatively larger phasor magnitudes than those obtained by the all-at-once technique.

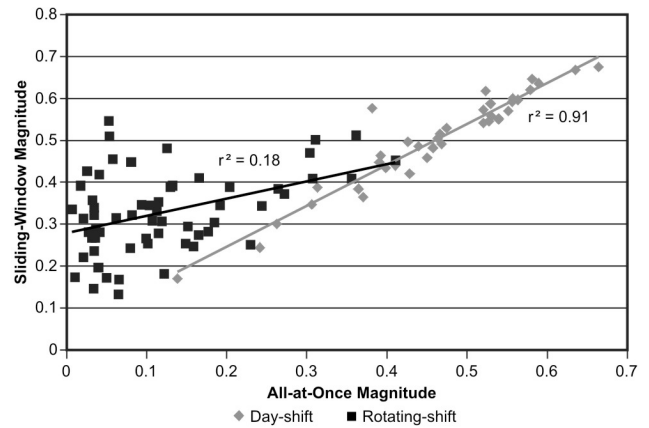


Figure 5: Comparison of phasor magnitudes for the sliding-window and the all-at-once techniques

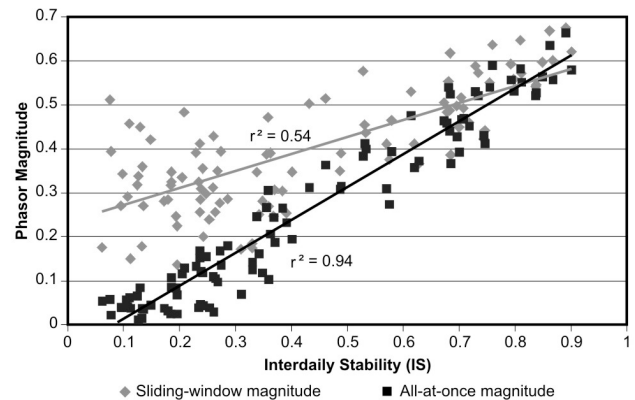


Figure 6: Comparison between the IS statistic based upon activity and the two techniques for determining phasor magnitude based on activity and light exposures

Figure 6 is a comparison of the IS statistic and the phasor magnitudes obtained using the sliding-window and the all-at-once techniques. The all-at-once technique yields results that correlate highly with the IS statistic ($r^2=0.94$). The IS statistic is inherently based upon an assumed 24-hour activity rhythm, but since it does not depend on light exposures, the high correlation indicates that light exposure maintained a similar pattern with respect to activity throughout the week. The relatively weaker correlation between the IS statistic and the sliding-window phasor magnitude implies that, although light and activity might be highly correlated, the period of oscillation did not conform precisely to a 24-hour period. That is, the 24-hour based IS statistic is low but the sliding-window phasor magnitude is high, relative to the all-at-once phasor magnitude. It is not known at this time which phasor technique is more predictive of health and well-being; must people maintain high regularity across all days (measured with the all-at-

once phasor) to be healthy or can people vary behavior (activity) across days (measured with the sliding-window phasor) without consequences to health and well-being?

Figure 7 illustrates sliding-window phasors for four different day-shift nurses paired with their average daily circadian stimulus (CS_A) and activity profiles. Because average activity and average light are plotted independent of one another, they are not strictly comparable to the corresponding phasors. Nevertheless, the paired diagrams do help illustrate how activity and light tend to affect phasor magnitudes and angles. Based upon examinations of a wide range of activity and light exposure profiles from day-shift nurses, the data from nurse A can be considered as “typical.” Generally speaking, a “typical” day-shift person exhibits a delayed phasor angle of between one and two hours with a phasor magnitude between 0.5 and 0.6. “Typical” individuals tend to be consistently active throughout their waking period, but are exposed to relatively higher light

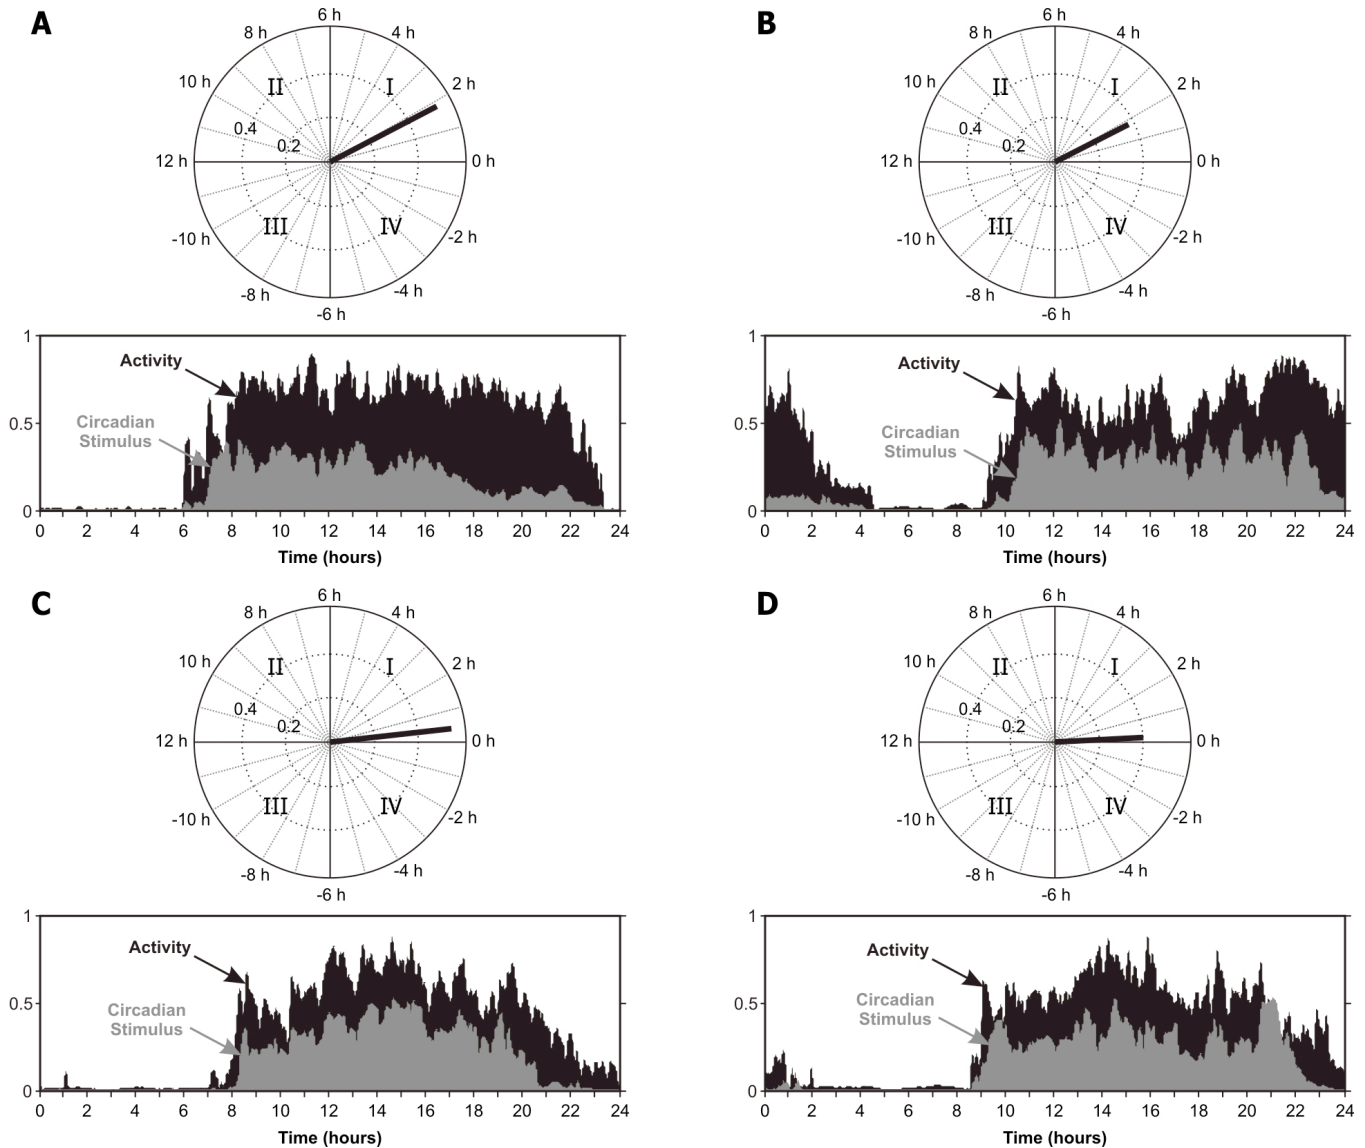


Figure 7: Average activity and average circadian stimulus (CS_A) values across a day with corresponding sliding-window phasors for four different day-shift nurses

levels in the early part of their activity period than toward the end. This asymmetry in relative light exposure from the early to the late part of their activity period, in fact, produces delayed phasor angles in Quadrant I. The phasor angle for the “typical” nurse is nearly the same as that for day-shift nurse B, but the phasor magnitude for nurse B is lower. Comparing the average activity and light exposure data for the two nurses, it is clear that for both nurses light exposures are lower in the late part of the activity period than in the early part of the activity period, thus leading to their nearly identical phasor angles. It is even clearer that activity is more variable and less well correlated with light exposure for nurse B than for nurse A. This yields a shorter phasor magnitude for nurse B than for nurse A. It is important to point out that the absolute time of activity and light do not affect the phasor angle or the phasor magnitude, at least not directly. Again, the phasor is based upon the synchronization between activity and actual light exposure, not between activity and clock time. The phasor magnitudes for nurses A and C are nearly identical, the major difference is in their phasor angles. It can be readily appreciated from this figure that nurse C does not exhibit the relative asymmetry in light exposure from the early to the late activity period as is seen with nurse A. Consequently the phasor angle for nurse C is advanced with respect to nurse A to near 0 hours. The average activity and light exposure data for nurse D are very much like those for nurse C except they are less well correlated, yielding the same phasor angle, but a lower phasor magnitude. Compared to the “typical” nurse A then, nurse D is more variable in her activity and light exposure patterns and does not exhibit the asymmetry of activity from the early to the late parts of her activity period. Of potential interest, nurse D appears to be exposed to bright light toward the end of her activity period relative to any of the other nurses, including the “typical” nurse. Also it should be noted that the period of time with no light and activity (presumably sleep) is less for nurses B and D than for nurses A and C who both have relatively large phasor magnitudes. Again, whether these differences are predictive of health and well-being remains to be studied systematically.

DISCUSSION

It is becoming clearer that human health and well-being are dependent upon the synchronization of biological systems [13]. The master clock in the SCN sets the pace for peripheral systems, but if these complex systems become asynchronous with one another (e.g., following jet lag) we experience poor sleep, indigestion, and performance errors. These, in turn, may lead to chronic problems such as insomnia, diabetes and obesity, and injury.

Since the pattern of light and dark drives the timing of the master clock, it is obviously important for our evolving understanding of human health that we begin to measure the light-dark cycles actually experienced by individuals in their own living environments as affected by electric lighting and modern day work schedules. The Daysimeter was developed for this purpose. Measuring the light-dark

patterns experienced by people in their living environments is important, but those data are not particularly valuable unless it is possible to interpret them in the context of human well-being and health. Phasor analysis was developed to quantify the synchronization of oscillating light-dark patterns and activity-rest patterns, thereby giving an individual-specific measure of behavioral circadian entrainment or disruption. In addition to activity, but not examined here, other measures of circadian regulated processes, such as core body temperature, heart rate, and hormone levels, can be made together with light exposure measurements and then analyzed using the phasor analysis technique described here.

It is also readily possible to relate individual-specific measures of circadian disruption to individual-specific measures of performance, affect and fatigue. It is also theoretically possible to develop individual-specific treatments to correct circadian disruption and measure their efficacy through changes in phasor magnitude and angle as they relate to changes in medically meaningful outcomes. Obviously genetic differences as well as differences in environmental stressors must also be considered. In the near future, however, it should be possible, using tools like the Daysimeter and phasor analysis, to begin to bridge ecological measurements of circadian disruption to controlled studies of circadian disruption using animal models for such diseases as cancer, cardiovascular disease, and diabetes.

Recently we were able to show the feasibility of this bridge. Figure 2 shows the circular correlations and associated phasors for a day-shift nurse and a rotating-shift nurse together with the circular correlations and associated phasors for a rat placed on a regular 12L:12D schedule and a rat placed on a regularly reversing (i.e., continuous jet lag) pattern of light and dark. As can readily be appreciated from Figure 2, and despite the differences in two species with regard to their photic niche (i.e., diurnal nurses versus nocturnal rats), it should now be possible to parametrically study the impact of circadian disruption actually experienced by individuals in different living environments with any one of several animal models for human diseases and disorders. These envisioned studies can then serve as the next logical step in understanding the impact of circadian disruption on human health, complementing the pioneering epidemiological studies that raised our collective concern for how circadian disruption might impact human health [17, 19].

ACKNOWLEDGEMENTS

This work was supported in part by CDC Grant 1R01 OH008171 to Dr. Eva Schernhammer at Harvard Public Health and by the Trans-NIH Genes, Environment and Health Initiative Grant 1U01 DA023822-01 to Dr. Mark Rea at the Lighting Research Center. The authors would like to thank Terry Klein and Dennis Guyon of the Lighting Research Center for their assistance with the study and manuscript.

REFERENCES

1. Bechtold, D.A. Energy-responsive timekeeping. *J Genet.* 2008 Dec;87(5):447-58.
2. Berson, D.M., Dunn, F.A., Takao, M. Phototransduction by retinal ganglion cells that set the circadian clock. *Science* 2002, 295:1070-1073.
3. Bierman, A., Klein, T.R., Rea, M.S. The Daysimeter: A device for measuring optical radiation as a stimulus for the human circadian system. *Measurement Science and Technology* 2005, 16:2292-2299.
4. Brainard, G.C., Hanifin, J.P., Greeson, J.M., Byrne, B., Glickman, G., Gerner, E., Rollag, M.D. Action spectrum for melatonin regulation in humans: Evidence for a novel circadian photoreceptor. *J. Neurosci.* 2001, 21(16):6405-6412.
5. Commission International de l'Eclairage (CIE). Light as a True Visual Quantity: Principles of Measurement. *Commission Internationale de l'Eclairage* 1978, Paris.
6. Erren, T. C. and Reiter, R.J. Defining chronodisruption. *J Pineal Res.* 2009 Apr: 46(3):245-7. Epub 2009 Feb 9.
7. Ingling, C.R., Martinez-Urieegas, E. The relationship between spectral sensitivity and spatial sensitivity for the primate r-g X-channel. *Vision Research* 1983, 23:1495-1500.
8. Kohsaka, A., Bass, J. A sense of time: How molecular clocks organize metabolism. *Trends Endocrinol Metab* 2007, 18(1):4-11.
9. Mallis, M.M., DeRoshia, C.W. Circadian rhythms, sleep, and performance in space. *Aviat Space Environ Med* 2005, 76(6 Suppl):B94-107
10. McIntyre, I., Norman, T.R., Burrows, G.D., Armstrong, S.M. Human melatonin suppression by light is intensity dependent. *J Pineal Research* 1989. 6(2):149-156.
11. Rea, M., Bierman, A., Figueiro, M., Bullough, J.D. A new approach to understanding the impact of circadian disruption on human health. *J Circ Rhy* 2008. 6:7.
12. Rea, M.S., Figueiro, M.G., Bullough, J.D., Bierman, A. A model of phototransduction by the human circadian system. *Brain Res Rev* 2005, 50(2):213-228.
13. Reddy, A.B., Wong, G.K., O'Neill, J., Maywood, E.S., Hastings, M.H. Circadian clocks: neural and peripheral pacemakers that impact upon the cell division cycle. *Mutat Res* 2005 Jul 1; 574(1-2):76-91. Epub 2005 Apr 15.
14. Reppert, S. M., and Weaver, D.R. Coordination of circadian timing in mammals. *Nature* 418, 935-941 (29 August 2002).
15. Sack, R.L., Auckley, D., Auger, R.R., Carskadon, M.A., Wright, K.P., Jr., Vitiello, M.V., Zhdanova, I.V. Circadian rhythm sleep disorders: part II, advanced sleep phase disorder, delayed sleep phase disorder, free-running disorder, and irregular sleep-wake rhythm. (An American Academy of Sleep Medicine review.) *Sleep* 2007, 30(11):1484-1501.
16. Schanda, J., Morren, L., Rea, M., Rositani-Ronchi, L., Walraven, P. Does lighting need more photopic luminous efficiency functions? *Lighting Res. Technol.* 2002. 34,1: 69-78.
17. Schernhammer, E.S., Laden, F., Speizer, F.E., Willett, W.C., Hunter, D.J., Kawachi, I. Rotating night shifts and risk of breast cancer in women participating in the Nurses' Health Study. *J Natl Cancer Inst* 2001, 93:1563-1568.
18. Smith, V.C., Pokorny, J. Spectral sensitivity of the foveal cone photopigments between 400 and 500 nm. *Vision Research* 1975, 15:161-171.
19. Stevens, R.G., Blask, D.E., Brainard, G.C., Hansen, J., Lockley, S.W., Provencio, I., Rea, M.S., Reinlib, L. Meeting report: the role of environmental lighting and circadian disruption in cancer and other diseases. *Environ Health Perspect* 2007, 115(9):1357-1362.
20. Straif, K., Baan, R., Grosse, Y., Secretan, B., Ghissassi, F.E., Bouvard, V., Altieri, A., Benbrahim-Tallaa, L., Cogliano, V. Carcinogenicity of shift-work, painting, and fire-fighting. *The Lancet Oncology* 2007, 8(12):1065.
21. Thapan, K., Arendt, J., Skene, D.J. An action spectrum for melatonin suppression: Evidence for a novel non-rod, non-cone photoreceptor system in humans. *J Physiol* 2001, 525(Pt 1):261-267.
22. Van Derlofske, J., Bierman, A., Rea, M.S., Ramanath, J., Bullough, J.D. Design and optimization of retinal flux density meter. *Meas. Sci. Technol.* 2002, 13:821.
23. Van Someren, E.J.W., Hagebeuk, E.E., Lijzenga, C., Scheltens, P., de Rooij, S.E., Jonker, C., Pot, A.M., Mirmiran, M., Swaab, D.F. Circadian rest-activity rhythm disturbances in Alzheimer's disease. *Biol Psychiatry* 1996, 40:259-270.
24. Young, M.E., and Bray, M.S. Potential role for peripheral circadian clock dyssynchrony in the pathogenesis of cardiovascular dysfunction. *Sleep Med* 2007. 8(6):656-67.
25. Zeitzer, J.M., Dijk, D.J., Kronauer, R., Brown, E., Czeisler, C. Sensitivity of the human circadian pacemaker to nocturnal light: melatonin phase resetting and suppression. *J Physiol* 2000, 526(Pt 3):695-702.